

AASHTO/AWS D1.5M/D1.5:2008
An American National Standard

Bridge Welding Code

A Joint Publication of
American Association of State Highway
and Transportation Officials



American Welding Society

second printing, June 2009

**AASHTO/AWS D1.5M/D1.5:2008
An American National Standard**

**Approved by the
American National Standards Institute
July 24, 2007**

Bridge Welding Code

5th Edition

Supersedes AASHTO/AWS D1.5M/D1.5:2002

Prepared by the
American Welding Society (AWS) D1 Committee on Structural Welding
AASHTO Highway Subcommittee on Bridges and Structures

Under the Direction of the
AWS Technical Activities Committee
AASHTO Executive Committee

Approved by the
AWS Board of Directors
AASHTO Board of Directors/Policy Committee

Abstract

This code covers the welding requirements for AASHTO welded highway bridges made from carbon and low-alloy constructional steels. This 2008 edition contains dimensions in metric SI Units and U.S. Customary Units. Clauses 1 through 7 constitute a body of rules for the regulation of welding in steel construction. The provisions for Clause 9 have been distributed throughout the D1.5 code. Clauses 8, 10, and 11 do not contain provisions, as their analogue D1.1 sections are not applicable to the D1.5 code. Clause 12 contains the requirements for fabricating fracture critical members.

A Joint Publication of:

**American Association of State
Highway and Transportation Officials**
444 N. Capitol Street, N.W., Suite 225
Washington, DC 20001

American Welding Society
550 N.W. LeJeune Road
Miami, FL 33126

Foreword

This foreword is not part of AASHTO/AWS D1.5M/D1.5:2008, *Bridge Welding Code*, but is included for informational purposes only.

The preparation of this specification was undertaken in response to a need for a common welding specification for the fabrication of steel highway bridges by welding. The departments of highways and transportation in the 50 states, the District of Columbia, and Puerto Rico that make up the American Association of State Highway and Transportation Officials have routinely used the specifications of the American Welding Society Structural Welding Committee, with appropriate modifications, to produce contract documents suitable for the construction of bridges using Federal Highway funds. The proliferation of requirements by the 50 states, District of Columbia and Puerto Rico that make up AASHTO (American Association of State Highway and Transportation Officials) resulted in the recognition of the need for a single document that could produce greater economies in bridge fabrication, while at the same time addressing the issues of structural integrity and public safety.

The first AWS code for *Fusion Welding and Gas Cutting in Building Construction* was published in 1928. In 1934, a committee was appointed to prepare specifications for the design, construction, alteration, and repair of highway and railway bridges. The first bridge specification was published in 1936. Until 1963, there were separate AWS committees for bridges and buildings. These two committees joined in 1963 to form the Structural Welding Committee of the American Welding Society. The committee has since promulgated standards for the application of welding to the design and construction of structures.

The Federal Highway Administration of the United States Department of Transportation requires states using federal funds for the construction of welded highway bridges to conform to specified standards for design and construction. Conformance to the AWS *Specification for Welded Highway and Railway Bridges* was first specified in the third edition of the AASHTO *Standard Specifications for Highway Bridges* in 1941. In 1962, the Bureau of Public Roads, now the Federal Highway Administration (FHWA), required conformance to a Circular Memorandum, dated November 13, 1962, which transmitted additional provisions for welding A36 steel pending publication of an AWS specification which would contain certain essential provisions not then in the code. Another Circular Memorandum, dated February 11, 1965, specified requirements for CVN testing, and a further Circular Memorandum, dated August 19, 1966, modified provisions of the 1966 Edition of the AWS D2.0-66, *Specification for Welded Highway and Railway Bridges*. An FHWA notice, dated July 7, 1971, recommended that ultrasonic inspection not be used for final acceptance of welds made by electrogas or electroslag procedures because of concern that the acceptance levels of AWS D2.0-69, Appendix C, were not suitable to detect or reject piping porosity of major dimensions.

In 1974, AASHTO published the first edition of the *Standard Specification for Welding of Structural Steel Highway Bridges*. The Eleventh Edition of the AASHTO *Standard Specifications for Highway Bridges*, dated 1977, directed “Welding shall conform to the requirements of the AASHTO *Standard Specifications for Welding of Structural Steel Highway Bridges* 1974 and subsequent interim specifications...” AASHTO published the Second and Third editions of the *Standard Specifications for Welding of Structural Steel Highway Bridges* in 1977 and 1981. All of the AASHTO specifications were required to be part of the Contract Documents as modifications or additions to the AWS *Structural Welding Code—Steel*. This was a cumbersome procedure.

In 1982, a subcommittee was formed jointly by AASHTO and AWS, with equal representation from both organizations, to seek accommodation between the separate and distinct requirements of bridge Owners and existing provisions of AWS D1.1. The *Bridge Welding Code* is the result of an agreement between AASHTO and AWS to produce a joint AASHTO/AWS *Structural Welding Code* for steel highway bridges that addresses essential AASHTO needs and makes AASHTO revisions mandatory.

The 1988 version of the *Bridge Welding Code* provided for the qualification of welding procedures by test to assure that weld had the strength, ductility, and toughness necessary for use in redundant structures. Nonredundant fracture critical bridge members were not provided for in the first edition of the code. While qualification of welding procedures is required, a major effort has been made to specify the minimum number of tests and the simplest tests that give reasonable assurance of required mechanical properties. Efforts are made to discourage individual States from requiring duplication of weld testing unless that testing is specified in the bid documents. Special attention is directed to avoidance of unnecessary hardening of base metal HAZs and the avoidance of hydrogen and other items that can lead to weld or base-metal cracking.

Consequently, while the D1.5-88 document has a superficial resemblance to D1.1 in its general format, there are significant differences that users should be aware of, among them the lack of provisions relating to statically loaded structures, tubular construction or the modification of existing structures. Users are encouraged to develop their own requirements for these applications or use existing documents (e.g., D1.1) with the appropriate modifications.

The publication of AASHTO/AWS D1.5M/D1.5:2008 was justified by the need to monitor, revise, and update code provisions based on the needs of AASHTO member states and industry. The following is a list of the major revisions in 2008 edition:

- (1) Addition of Commentary for Clauses 2, 3, 4, 5, 6, and Annex G.
- (2) Deletion of material M270M [M270] Gr. 485W [70W] and inclusion of Gr. HPS 485W [HPS 70W].
- (3) Addition of a new normative annex detailing welding requirements for M270M/M270 [A709M/A709] Gr. HPS 485W [HPS 70W].
- (4) Inclusion of HPS 50W materials.
- (5) Addition of optional supplemental moisture-resistant designators.
- (6) Machining and testing tolerances for performance test specimens.
- (7) Additions and revisions to usage, handling, and storage requirements for consumables in fracture critical applications.
- (8) Revisions to Tables 4.1, 4.2, 4.4, and 4.5.
- (9) Addition of new filler metal variable in Table 5.3.
- (10) Revision to inspection personnel qualification.
- (11) Revised sample forms for WPSs and PQRs.

Changes in Code Requirements. Changes to the text of the 2008 edition are indicated by underlining. Changes to illustrations are highlighted by vertical lines in the margin.

Future revisions to this code will be made based on proposals from the Joint AASHTO/AWS Committee as well as those from document users. It should be re-emphasized here that the Joint Committee is the primary agency for receiving feedback from industry, and requires this input in order to produce a quality document. Other documents that do not receive the ANSI/AASHTO/AWS accreditation should not be relied on as substitutes for the Joint Committee's interpretation of D1.5 provisions.

While the D1.1 and D1.5 codes do share a number of common provisions, it should not be assumed that revisions to one document provision automatically revises its analogous provision in the other; therefore, users are encouraged to treat each code as an independent document.

This code was prepared by the AASHTO/AWS Bridge Welding Committee operating as a Subcommittee of the AWS Structural Welding Committee. The Committee is made up of representatives from the AWS Structural Welding Committee and the AASHTO Technical Committee for Welding. Accommodation was sought on all items where there was disagreement between AASHTO and AWS members. Specific issues considered essential by AASHTO were included in this code to eliminate the need for supplemental exclusions or additions by AASHTO.

The AASHTO/AWS D1.5, *Bridge Welding Code*, will be subject to regular review by the Bridge Welding Committee and will be republished or reaffirmed on an as-needed basis, at intervals not to exceed five years. All proposed changes to this code will be subject to approval by AWS and AASHTO prior to publication.

Comments or inquiries pertaining to this code are welcome (see Annex M). They should be sent to the Secretary, AWS D1 Committee on Structural Welding, American Welding Society, 550 N.W. LeJeune Road, Miami, FL 33126, or to the Chairman of the AASHTO Technical Committee for Welding, American Association of State Highway and Transportation Officials, 444 N. Capitol Street, N.W., Suite No. 225, Washington, DC 20001.


Errata

The following Errata have been identified and incorporated into the current reprint of this document.

Page 89—Clause 5.10.2—Delete paragraph after the “Fillet Weld Properties” title so that no verbiage exists in the clause.


Page 262—Form L-3 Procedure Qualification Records (PQR) for Qualification, Pretest, and Verification Results—Change “Maximum Size Single Pass” to “Minimum Size Multiple Pass” under Macroetch row.

Page 319—Figure C-3.5 (A) & (B) Illustration of Camber Tolerances for Steel Beams—For sketches (A) & (B) the line depicting the “Detailed Camber Shape” was corrected and made bolder than the line depicting “Actual Camber of the Steel” for additional clarity. Please see corrected figure below:

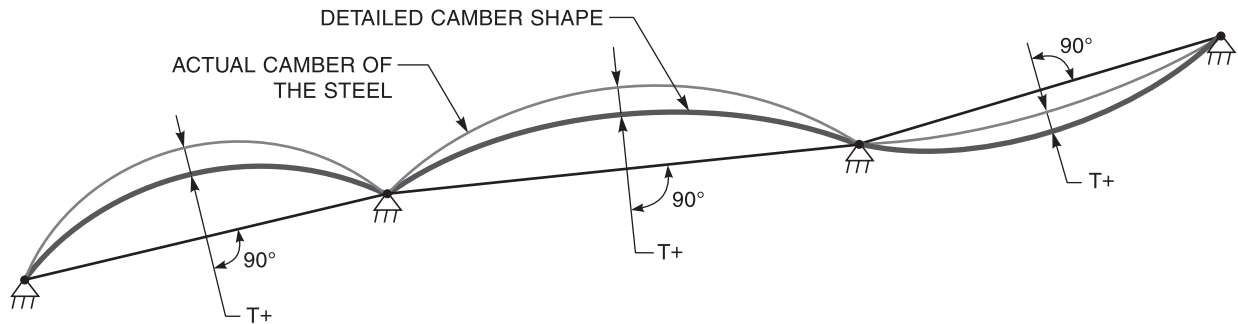

PLUS CAMBER TOLERANCE (T+) APPLIES WHEN THE ACTUAL CAMBER OF THE STEEL IS ABOVE THE DETAILED CAMBER SHAPE. THIS TOLERANCE IS MEASURED PERPENDICULAR TO A STRAIGHT LINE BETWEEN THE SUPPORTS OF EACH SPAN.

(A) PLUS CAMBER TOLERANCE

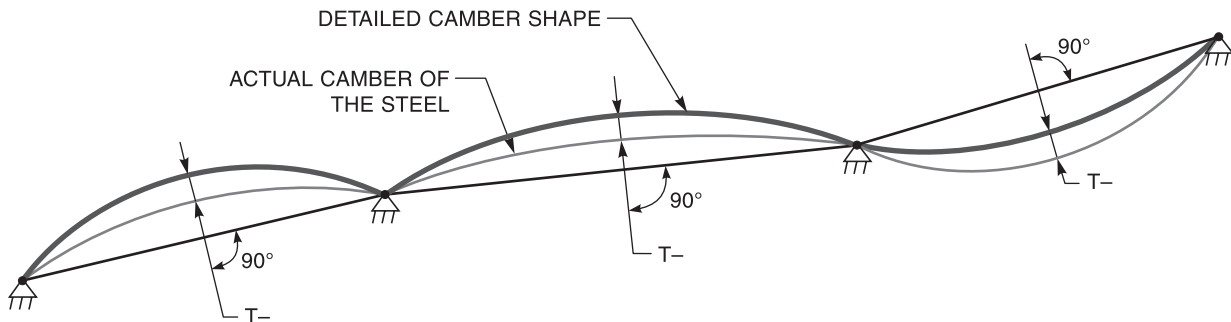

MINUS CAMBER TOLERANCE (T-) APPLIES WHEN THE ACTUAL CAMBER OF THE STEEL IS BELOW THE DETAILED CAMBER SHAPE. THIS TOLERANCE IS MEASURED PERPENDICULAR TO A STRAIGHT LINE BETWEEN THE SUPPORTS OF EACH SPAN.

(B) MINUS CAMBER TOLERANCE

Figure C-3.5—Illustration of Camber Tolerances for Steel Beams

Table of Contents

	Page No.
<i>Personnel</i>	v
<i>Foreword</i>	ix
<i>List of Tables</i>	xviii
<i>List of Figures</i>	xix
<i>List of Forms</i>	xxi
1. General Provisions	1
1.1 Application.....	1
1.2 Base Metal.....	1
1.3 Welding Processes.....	1
1.4 Fabricator Requirements.....	2
1.5 Definitions.....	2
1.6 Welding Symbols.....	2
1.7 Safety Precautions.....	2
1.8 Standard Units of Measurement.....	2
1.9 Welding Procedure Specifications (WPSs).....	3
1.10 Mechanical Testing.....	3
1.11 Reference Documents.....	3
2. Design of Welded Connections	5
Part A—General Requirements.....	5
2.1 Drawings.....	5
2.2 Basic Unit Stresses.....	6
2.3 Effective Weld Areas, Lengths, Throats, and Sizes.....	6
Part B—Structural Details.....	6
2.4 General.....	6
2.5 Welded Filler Plates.....	6
2.6 PJP Groove Welds.....	7
Part C—Details of Welded Joints.....	7
2.7 Joint Qualification.....	7
2.8 Details of Fillet Welds.....	7
2.9 Details of Plug and Slot Welds.....	7
2.10 Lap Joints.....	8
2.11 Corner and T-Joints.....	8
2.12 CJP Groove Welds.....	8
2.13 PJP Groove Welds.....	8
2.14 Prohibited Types of Joints and Welds.....	9
2.15 Combinations of Welds.....	9
2.16 Welds in Combination with Rivets and Bolts.....	9
2.17 Connection Details.....	9
3. Workmanship	51
3.1 General Requirements.....	51
3.2 Preparation of Base Metal.....	51
3.3 Assembly.....	54

3.4	Control of Distortion and Shrinkage	56
3.5	Dimensional Tolerances	56
3.6	Weld Profiles	58
3.7	Repairs	58
3.8	Peening.....	59
3.9	Caulking.....	60
3.10	Arc Strikes	60
3.11	Weld Cleaning	60
3.12	Weld Termination	60
3.13	Weld Backing	60
4.	Technique	65
	Part A—General Requirements	65
4.1	Filler Metal Requirements	65
4.2	Preheat and Interpass Temperature Requirements.....	66
4.3	Heat Input Control for Grade 690 [100] and 690W [100W]	67
4.4	Stress Relief Heat Treatment	67
	Part B—Shielded Metal Arc Welding (SMAW)	67
4.5	Electrodes for SMAW	67
4.6	Procedures for SMAW.....	68
	Part C—Submerged Arc Welding (SAW).....	69
4.7	General Requirements.....	69
4.8	Electrodes and Fluxes for SAW.....	69
4.9	Procedures for SAW with a Single Electrode.....	70
4.10	Procedures for SAW with Parallel Electrodes.....	70
4.11	Procedures for SAW with Multiple Electrodes	71
	Part D—Gas Metal Arc Welding (GMAW) and Flux Cored Arc Welding (FCAW)	72
4.12	Electrodes.....	72
4.13	Shielding Gas.....	73
4.14	Procedures for GMAW and FCAW with a Single Electrode	73
	Part E—Electroslag Welding (ESW) and Electrode Gas Welding (EGW).....	73
4.15	Qualification of Process, WPSs, and Joint Details	73
4.16	Mechanical Properties.....	74
4.17	Condition of Electrodes and Guide Tubes	74
4.18	Shielding Gas.....	74
4.19	Condition of Flux.....	74
4.20	Procedures for ESW and EGW	74
	Part F—Plug and Slot Welds	74
4.21	Plug Welds	74
4.22	Slot Welds.....	75
4.23	Plug and Slot Welds.....	75
	Part G—Control of Production Welding Variables	75
4.24	Tests	75
4.25	Control of Variables.....	75
4.26	Calibration of Equipment.....	75
4.27	Current Control	75
5.	Qualification	85
5.0	Scope.....	85
	Part A—Welding Procedure Specification (WPS) Qualification	85
5.1	Approval	85

	Page No.
5.2	Qualification Responsibility 85
5.3	Duration 85
5.4	Base Metal 86
5.5	Welding Consumables 87
5.6	Test Plate Thickness 87
5.7	General Requirements for WPS Qualification..... 87
5.8	Position of Test Welds 88
5.9	Options for WPS Qualification or Prequalification 89
5.10	Fillet Weld WPS Qualification 89
5.11	Prequalified WPS..... 89
5.12	Heat Input WPS 89
5.13	Production Procedure WPS 90
5.14	ESW and EGW 91
5.15	Type of Tests and Purpose..... 91
5.16	Weld Specimens—Number, Type, and Preparation 91
5.17	Nondestructive Testing (NDT) 92
5.18	Method of Testing Specimens 92
5.19	Test Results Required 93
5.20	Retests 93
Part B—Welder, Welding Operator, and Tack Welder Qualification 94	
5.21	General Requirements..... 94
5.22	Production Welding Positions Qualified 94
5.23	Qualification Tests Required 95
5.24	Limitations of Variables 96
5.25	Test Specimens: Number, Type, and Preparation..... 97
5.26	Method of Testing Specimens 97
5.27	Test Results Required 98
5.28	Retests 99
6.	Inspection 133
Part A—General Requirements 133	
6.1	General..... 133
6.2	Inspection of Materials 134
6.3	Inspection of WPS Qualification and Equipment..... 134
6.4	Inspection of Welder, Welding Operator, and Tack Welder Qualifications..... 134
6.5	Inspection of Work and Records 134
6.6	Obligations of the Contractor 135
6.7	Nondestructive Testing (NDT) 135
Part B—Radiographic Testing (RT) of Groove Welds in Butt Joints 137	
6.8	Extent of Testing..... 137
6.9	General..... 137
6.10	RT Procedure 137
6.11	Acceptability of Welds 140
6.12	Examination, Report, and Disposition of Radiographs 140
Part C—Ultrasonic Testing (UT) of Groove Welds 140	
6.13	General..... 140
6.14	Extent of Testing..... 140
6.15	UT Equipment..... 140
6.16	Reference Standards 141
6.17	Equipment Qualification..... 141
6.18	Calibration for Testing..... 141
6.19	Testing Procedures..... 142

6.20	Preparation and Disposition of Reports	143
6.21	Calibration of the UT Unit with IIW or Other Approved Reference Blocks	143
6.22	Equipment Qualification Procedures	144
6.23	Flaw Size Evaluation Procedures	146
6.24	Scanning Patterns.....	146
6.25	Examples of dB Accuracy Certification	146
	Part D—Weld Acceptance Criteria.....	146
6.26	Quality of Welds.....	146
7.	Stud Welding	167
7.1	Scope.....	167
7.2	General Requirements.....	167
7.3	Mechanical Requirements.....	167
7.4	Workmanship.....	168
7.5	Technique.....	168
7.6	Stud Application Qualification Requirements	169
7.7	Production Control.....	170
7.8	Inspection Requirements.....	171
8.	Statically Loaded Structures (No Applications within this code).....	175
9.	Welded Steel Bridges <u>(The provisions of this clause in ANSI/AASHTO/AWS [D1.5-96] were distributed throughout AASHTO/AWS [D1.5M/D1.5:2002] and remain so for this edition)</u>	177
10.	Tubular Structures (No Applications within this code).....	179
11.	Strengthening and Repairing Existing Structures (No Applications within this code).....	181
12.	AASHTO/AWS Fracture Control Plan (FCP) for Nonredundant Members	183
12.1	General Provisions	183
12.2	Definitions	183
12.3	Contract Documents	183
12.4	Base Metal Requirements	184
12.5	Welding Processes	184
12.6	Consumable Requirements	184
12.7	Welding Procedure Specification (WPS)	188
12.8	Certification and Qualification	188
12.9	As-Received Inspection of Base Metal.....	189
12.10	Thermal Cutting	189
12.11	Repair of Base Metal	189
12.12	Straightening, Curving, and Cambering	190
12.13	Tack Welds and Temporary Welds	190
12.14	Preheat and Interpass Temperature Control.....	190
12.15	Postweld Thermal Treatments	190
12.16	Weld Inspection	191
12.17	Repair Welding	192
	<i>Annexes</i>	197
	<u>Cross Reference for Renumbered Annexes from the 2002 Code to the 2008 Code</u>	198
	Annex <u>A</u> (Normative)—Effective Throat	199
	Annex <u>B</u> (Normative)—Effective Throats of Fillet Welds in Skewed T-Joints	201
	Annex <u>C</u> (Normative)—Flatness of Girder Webs—Bridges.....	203
	Annex <u>D</u> (Normative)—Terms and Definitions.....	209
	Annex <u>E</u> (Normative)—Manufacturer’s Stud Base Qualification Requirements	217

Page No.

Annex <u>F</u> (Normative)—Part A—Qualification and Calibration of the UT Unit with Other Approved Reference Blocks	221
Part B—UT Equipment Qualification Procedures.....	223
Annex <u>G</u> (Normative)—Guidelines on Alternative Methods for Determining Preheat.....	231
<u>Annex H</u> (Normative)— <u>Welding Requirements for Conventional, Nonfracture Critical M270M [M270] (A 709M [A 709]) HPS 485W [HPS 70W] Components with Reduced Preheat and Interpass Temperature</u>	241
Annex <u>I</u> (Informative)—Weld Quality Requirements for Tension Joints.....	243
Annex <u>J</u> (Informative)—Description of Common Weld and Base Metal Discontinuities.....	245
Annex <u>K</u> (Informative)—Short Circuiting Transfer.....	255
Annex <u>L</u> (Informative)—Suggested Sample Welding Forms	259
Annex <u>M</u> (Informative)—Guidelines for Preparation of Technical Inquiries for the Joint AASHTO/AWS Subcommittee on Bridge Welding.....	267
Annex <u>N</u> (Informative)—Reference Documents.....	269
<i>Commentary on Bridge Welding Code</i>	271
Foreword.....	273
Index	395
List of AWS Documents on Structural Welding.....	409

List of Tables

Table	Page No.
2.1	Minimum Fillet Weld Size..... 11
2.2	Minimum Effective Weld Size for PJP Groove Welds..... 11
3.1	Limits on Acceptability and Repair of Cut Edge Discontinuities of Material..... 62
3.2	Camber Tolerance for Typical Girder..... 62
3.3	Camber Tolerance for Girders without a Designed Concrete Haunch..... 62
4.1	Matching Filler Metal Requirements for WPSs Qualified in Conformance with 5.12..... 76
4.2	Matching Filler Metal Requirements for WPSs Qualified in Conformance with 5.13..... 79
4.3	Filler Metal Requirements for Exposed Bare Application of M270M [M270] (A709M [A709]) Gr. 345W [50W] and Gr. HPS 345W [HPS 50W] Steel..... 82
4.4	Minimum Preheat and Interpass Temperature, °C [°F] 82
4.5	Minimum Holding Time 83
4.6	Alternate Stress-Relief Heat Treatment 83
4.7	Allowable Atmospheric Exposure of Low-Hydrogen SMAW Electrodes 83
5.1	WPS Qualification Requirements for Consumables 100
5.2	WPS Qualification or Prequalification Options 100
5.3	PQR Essential Variable Changes for WPSs Qualified per 5.13.3 101
5.4	Additional PQR Essential Variable Changes Requiring WPS Requalification for ESW or EGW..... 104
5.5	Required Number of Test Specimens—WPS Qualification 105
5.6	Welder Qualification—Type and Position Limitations 105
5.7	Number and Type of Specimens and Range of Thickness Qualified—Welder and Welding Operator Qualification..... 106
6.1	Hole-Type IQI Requirements..... 149
6.1A	Wire IQI Requirements 149
6.2	Testing Angle 150
6.3	UT Acceptance-Rejection Criteria—Tensile Stress..... 152
6.4	UT Acceptance-Rejection Criteria—Compressive Stress..... 153
7.1	Mechanical Property Requirements for Studs..... 172
7.2	Minimum Fillet Weld Size for Small Diameter Studs 172
12.1	CVN Test Values of Weld Metal with Matching Strength 194
12.2	Tack Weld Requirements 194
12.3	M270M [M270] (A709M [A709]) Gr. 250 [36], 345 [50] Minimum Preheat and Interpass Temperatures, °C [°F] 195
12.4	M270M [M270] (A709M [A709]) Gr. 345W [50W], HPS 345W [HPS 50W], HPS 485W [HPS 70W] Minimum Preheat and Interpass Temperatures, °C [°F] 195
12.5	M270M [M270] (A709M [A709]) Gr. 690 [100], 690W [100W] Minimum and Maximum Preheat/Interpass Temperatures, °C [°F]..... 195
<u>B.1</u>	Equivalent Fillet Weld Leg Size Factors for Skewed T-Joints, R = 0 202
<u>G.1</u>	Susceptibility Index Grouping as Function of Hydrogen Level “H” and Composition Parameter P _{cm} 234
<u>G.2</u>	Minimum Preheat and Interpass Temperatures for Three Levels of Restraint 234
<u>H.1</u>	Minimum Preheat and Interpass Temperature for M270M [M270] (A709M [A709]) HPS 485W [HPS 70W], °C [°F] 242
<u>H.2</u>	Filler Metals for Use with the Reduced Preheat of Table H.1, Diffusible Hydrogen Levels 4 mL/100 g Maximum..... 242
<u>J.1</u>	Common Types of Discontinuities..... 249
<u>K.1</u>	Typical Current Ranges for Short Circuiting Transfer Gas Metal Arc Welding (GMAW-S) of Steel 256

List of Figures

Figure		Page No.
2.1	Filler Plates Less Than 6 mm [1/4 in] Thick.....	12
2.2	Filler Plates 6 mm [1/4 in] or Thicker.....	12
2.3	Details for Fillet Welds	13
2.4	Details of Welded Joints for CJP Groove Welds	15
2.5	Details of Welded Joints for PJP Groove Welds.....	35
2.6	Fillet Welds on Opposite Sides of a Common Plane of Contact	47
2.7	Transition of Thickness at Butt Joints of Parts Having Unequal Thickness	48
2.8	Transition of Width at Butt Joints of Parts Having Unequal Width	49
3.1	Discontinuities in Cut Plate.....	63
3.2	Workmanship Tolerances in Assembly of Groove Welded Joints	63
3.3	Acceptable and Unacceptable Weld Profiles	64
4.1	Weld Bead in Which Depth and Width Exceed the Width of the Weld Face.....	84
5.1	WPS Qualification or Pretest—Test Plate A.....	107
5.2	WPS Verification—Test Plate B	108
5.3	Weld Soundness Test Plate for Details Not Conforming to Figure 2.4 or 2.5—Test Plate C	109
5.4	Positions of Fillet Welds	111
5.5	Positions of Groove Welds.....	111
5.6	Position of Test Plates for Groove Welds	112
5.7	Position of Test Plates for Fillet Welds.....	113
5.8	Fillet Weld Soundness Test (Macroetch) for WPS Qualification—Test Plate D	114
5.9	Standard Round All-Weld-Metal Tension Specimen.....	115
5.10	Reduced Section Tension Specimen	115
5.11	Side-Bend Specimen	116
5.12	Face- and Root-Bend Specimen	116
5.13	CVN Test Specimen—Type A.....	117
5.14	Guided Bend Test Jig	118
5.15	Alternative Wraparound Guided Bend Test Jig	119
5.16	Alternative Roller-Equipped Guided Bend Test Jig for Bottom Ejection of Test Specimen	120
5.17	Test Plate for Unlimited Thickness—Welder Qualification	121
5.18	Optional Test Plate for Unlimited Thickness—Horizontal Position—Welder Qualification	122
5.19	Test Plate for Limited Thickness—All Positions—Welder Qualification.....	123
5.20	Optional Test Plate for Limited Thickness—Horizontal Position—Welder Qualification	123
5.21	Fillet-Weld-Break and Macroetch Test Plate—Welder Qualification—Option 1.....	124
5.22	Fillet Weld Root-Bend Test Plate—Welder Qualification—Option 2	125
5.23	Plug Weld Macroetch Test Plate—Welder Qualification	126
5.24	Test Plate for Unlimited Thickness—Welding Operator Qualification	127
5.25	Butt Joint for Welding Operator Qualification—ESW and EGW	128
5.26	Fillet-Weld-Break and Macroetch Test Plate—Welding Operator Qualification—Option 1	129
5.27	Fillet Weld Root Bend Test Plate—Welding Operator Qualification—Option 2	130
5.28	Fillet-Weld-Break Specimen—Tack Welder Qualification	131
5.29	Method of Rupturing Specimen—Tack Welder Qualification	131
6.1A	Radiographic Identification and Hole-Type or Wire IQI Locations on Approximately Equal Thickness Joints 250 mm [10 in] and Greater in Length.....	154

Figure	Page No.
6.1B	Radiographic Identification and Hole-Type or Wire IQI Locations on Approximately Equal Thickness Joints Less than 250 mm [10 in] in Length 154
6.1C	Radiographic Identification and Hole-Type or Wire IQI Locations on Transition Joints 250 mm [10 in] and Greater in Length 155
6.1D	Radiographic Identification and Hole-Type or Wire IQI Locations on Transition Joints Less than 250 mm [10 in] in Length 155
6.1E	Hole-Type IQI Design 156
6.1F	Wire-Type IQI 157
6.2	RT Edge Block Placement 158
6.3	Transducer Crystal 159
6.4	Qualification Procedure of Search Unit Using IIW Reference Block 159
6.5A	International Institute of Welding (IIW) UT Reference Blocks 160
6.5B	Other Approved UT Reference Blocks 161
6.6	Transducer Positions (Typical) 163
6.7	Plan View of UT Scanning Patterns 164
6.8	Weld Quality Requirements for Discontinuities Occurring in Tension Welds (Limitations of Porosity and Fusion Discontinuities) 165
6.9	Weld Requirements for Discontinuities Occurring in Compression Welds (Limitations of Porosity or Fusion Type Discontinuities) 166
7.1	Dimension and Tolerances of Standard-Type Shear Connectors 173
7.2	Typical Tension Test Fixture 173
7.3	Torque Testing Arrangement and Table of Testing Torques 174
<u>E.1A</u>	Bend Testing Device 219
<u>E.1B</u>	Suggested Type of Device for Qualification Testing of Small Studs 219
<u>F.1</u>	Example of the Use of Form <u>F-1</u> UT Unit Certification 224
<u>F.2</u>	Example of Form <u>F-2</u> 225
<u>F.3</u>	Example of the Use of Form <u>F-2</u> 226
<u>F.4</u>	Example of Form <u>F-3</u> 227
<u>F.5</u>	Example of the Use of Form <u>F-3</u> 228
<u>F.6</u>	Form <u>F-4</u> —Report of UT of Welds 229
<u>G.1</u>	Zone Classification of Steels 235
<u>G.2</u>	Critical Cooling Rate for 350 <u>HV</u> and 400 <u>HV</u> 236
<u>G.3</u>	Charts to Determine Cooling Rates for Single-Pass Submerged Arc Fillet Welds 237
<u>G.4</u>	Relation Between Fillet Weld Size and Energy Input 240
<u>J.1</u>	Weld in Butt Joint 250
<u>J.2</u>	Weld in Corner Joint 251
<u>J.3</u>	Weld in T-Joint 252
<u>J.4</u>	Weld in Lap Joint 253
<u>J.5</u>	Single-Pass Fillet Weld in T-Joint 253
<u>J.6</u>	Single-V-Groove Weld in Butt Joint 254
<u>K.1</u>	Oscillograms and Sketches of Short Circuiting Arc Metal Transfer 257
<i>Commentary</i>	
<u>C-2.1</u>	<u>Details of Alternative Groove Preparations for Corner Joint</u> 294
<u>C-3.1</u>	Examples of Unacceptable Reentrant Corners 317
<u>C-3.2</u>	Examples of Good Practice for Cutting Copcs 317
<u>C-3.3</u>	<u>Permissible Offset in Abutting Members</u> 318
<u>C-3.4</u>	<u>Correction of Misaligned Members</u> 318
<u>C-3.5</u>	<u>Illustration of Camber Tolerances for Steel Beams</u> 319
<u>C-3.6</u>	<u>Measurement of Flange Warpage and Tilt</u> 320
<u>C-3.7</u>	<u>Tolerances Bearing Points</u> 321

List of Forms

Form		Page No.
<u>L-1</u>	Certificate of Conformance to Requirements for Welding Electrodes	260
<u>L-2</u>	Sample Welding Procedure Specification.....	261
<u>L-3</u>	Procedure Qualification Record (PQR) for Qualification, Pretest, and Verification Results	262
<u>L-4</u>	<u>Procedure Qualification Record (PQR) Worksheet</u>	263
<u>L-5</u>	Welder and Welding Operator Qualification Record.....	264
<u>L-6</u>	Report of Radiographic Examination of Welds	265
<u>L-7</u>	Report of Magnetic Particle Examination of Welds	266

Bridge Welding Code

1. General Provisions

1.1 Application

1.1.1 This code covers welding fabrication requirements applicable to welded highway bridges. It is to be used in conjunction with the *AASHTO Standard Specification for Highway Bridges* or the *AASHTO LRFD Bridge Design Specifications*.

The code is not intended to be used for the following:

- (1) Steels with a minimum specified yield strength greater than 690 MPa [100 ksi]
- (2) Pressure vessels or pressure piping
- (3) Base metals other than carbon or low alloy steels
- (4) Structures composed of structural tubing

Fabrication of structures or components not specifically addressed by this code shall be performed in conformance with the special provisions of the contract or in conformance with the written directives of the Engineer who may choose to reference an alternate applicable welding standard.

1.1.2 The fundamental premise of the code is to provide general stipulations applicable to any routine bridge situation. Acceptance criteria for production welds different from those described in the code may be used for a particular application, provided they are suitably documented by the proposer and approved by the Engineer.

Such alternate acceptance criteria may be based upon evaluation of suitability for service using past experience, experimental evidence, or engineering analysis considering material type, service load effects, and environmental factors.

1.1.3 The term *Engineer* as used in this code shall mean the State Bridge Engineer, or the Bridge Engineer's designated representative. The Engineer acts on behalf of the State or Owner and unless otherwise specified, shall be the Owner's official representative. All references to acceptance or approval shall mean acceptance or approval by the Engineer.

1.1.4 The term *Contractor* as used in this code indicates the party responsible for performing the work as required by the contract documents. The term Contractor is used collectively to mean contractor, manufacturer, fabricator, erector, or other party performing the work.

1.2 Base Metal

1.2.1 Specified Base Metal. The contract documents shall designate the specification and classification of base metals to be used.

1.2.2 Approved Base Metals. Unless otherwise specified, base metals to be welded under this code shall meet the requirements of the latest edition of AASHTO M270M [M270] (ASTM A 709M [A 709]) for the grade of steel shown on the plans or described in the specifications. All Grade 345 (50) steel that is to be welded shall be Type 1, 2, or 3. Other steels may be approved by the Engineer. Thickness limitations shall not apply to bearing components.

M270M [M270] steels of a designated grade are essentially the same as ASTM A 709M [A 709] steels of the same grade. The provisions of this code are not intended for use with steels having a minimum specified yield strength over 690 MPa [100 ksi].

1.2.3 Thickness Limitations. The provisions of this code do not apply to welding base metals less than 3 mm [1/8 in] thick. Where base metals thinner than 3 mm [1/8 in] are to be welded, the requirements of AWS D1.3/D1.3M, *Structural Welding Code—Sheet Steel*, should apply. When used in conjunction with AWS D1.3/D1.3M, the applicable provisions of this code shall be observed.

1.3 Welding Processes

1.3.1 Shielded metal arc welding (SMAW) WPSs (Welding Procedure Specifications) which conform to the provisions of Clauses 2, 3, and 4, are operated within the